


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130142 ✓</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Scott Gardner</u>	ID# <u>6222 ✓</u> Date <u>12 Oct 2010 ✓</u>
A Agency <u>Directorate of Emergency Services (FRN4)</u> Phone # <u>907-384-3888</u>	
Instrument Location <u>Bldg 656 A St Ft Richardson, AK</u>	
B Alco S/N <u>31085 ✓</u> Target Value <u>.074 ✓</u> High Pressure <u>300</u>	
Alco Test Values <u>.075 ✓</u> <u>.076 ✓</u>	
1st Alco 2nd Alco	
Signature <u></u>	
(OVER)	


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

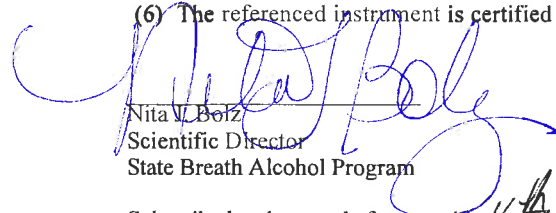
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 16th day of DEC, 2010.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



BMB
12/16/10

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130142 BMB 12/16/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

OCTOBER 12, 2010

OPERATOR'S NAME:

GARDNER/SCOTT/E

OPERATOR'S NUMBER: 6222

SUBJECT'S LAST NAME:

N/A

SUBJECT'S FIRST NAME/MI :

N/A

O.L. #: VERIFICATION OF CAL

DEPT/AGENCY: FR/4

CASE/REPORT: N/A

TEST TYPE: U

ALCO TARGET VALUE: .074

ALCO S/N: 31085

--- BREATH ANALYSIS ---

.074 ADJUSTED FOR 29.51 in

ALCO TARGET .072 13:49

BLANK TEST .000 13:50

INTERNAL STANDARD VERIFIED 13:50

ALCO TO 29.51 in .075 13:50

BLANK TEST .000 13:51

SUBJECT SAMPLE .000 13:51

BLANK TEST .000 13:52

ALCO TO 29.51 in .076 13:52

BLANK TEST .000 13:53

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130142

OCTOBER 12, 2010
TIME 13:47

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 03/29/00

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 45c

BAROMETER: 29.51 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~■